

**ENGLISH**


# **User manual**



**Table of contents:**

1. PRECAUTIONS AND SAFETY MEASURES .....	2
1.1. Preliminary instructions .....	2
1.2. During use .....	2
1.3. After use .....	2
2. GENERAL DESCRIPTION .....	3
3. PREPARATION FOR USE .....	3
3.1. Initial checks .....	3
3.2. Instrument power supply .....	3
3.3. Storage .....	3
4. NOMENCLATURE .....	4
4.1. Instrument description .....	4
4.2. Display description .....	4
4.3. Description of function keys .....	5
4.3.1. ON/OFF key .....	5
4.3.2. LX/FC/CD key .....	5
4.3.3. HLD key .....	5
4.3.4. MEM/READ key .....	5
4.3.5. Deleting the internal memory .....	5
4.3.6. MAXMIN key .....	5
4.3.7. ZRO key .....	5
4.3.8. ☀/SRC (Light Source) key .....	6
4.3.9. Disabling the Auto Power OFF function .....	6
5. OPERATING INSTRUCTIONS .....	7
5.1. Illuminance measurement .....	7
5.2. Luminous intensity measurement .....	7
6. MAINTENANCE .....	8
6.1. Battery replacement .....	8
6.2. Cleaning the instrument .....	8
6.3. End of life .....	8
7. TECHNICAL SPECIFICATIONS .....	9
7.1. Technical characteristics .....	9
7.1.1. Spectrum response .....	9
7.1.2. Sensor .....	9
7.1.3. General characteristics .....	10
7.2. Environment .....	10
7.2.1. Environmental conditions for use .....	10
7.3. Accessories .....	10
7.3.1. Accessories provided .....	10
8. SERVICE .....	11
8.1. Warranty conditions .....	11
8.2. Service .....	11

## 1. PRECAUTIONS AND SAFETY MEASURES

The instrument has been designed in compliance with the safety directives relevant to electronic measuring instruments. In order to prevent damaging the instrument, please carefully follow the procedures described in this manual and read all notes preceded by the symbol  with the utmost attention. Before and after carrying out the measurements, carefully observe the following instructions:


- Do not carry out any measurements in case gas, explosive materials or flammables are present, or in dusty environments
- Do not carry out any measurement in humid environments
- Do not carry out any measurement in case you find anomalies such as deformation, breaks, substance leaks, absence of display on the screen, etc.
- Do not touch the photodiode sensor while carrying out measurements, in order to prevent any damage to the instrument caused by static electricity or contamination

The following symbol is used in this manual:



Caution: observe the instructions given in this manual. Improper use could damage the instrument and/or its components.

### 1.1. PRELIMINARY INSTRUCTIONS

In order to prevent incorrect reading, replace the battery when the symbol "" appears on the display when switching on the instrument.

### 1.2. DURING USE

Please carefully read the following recommendations and instructions.



#### CAUTION

Failure to comply with the Caution notes and/or Instructions may damage the instrument and/or its components or be a source of danger for the operator.

While measuring, if the value or the sign of the quantity being measured remain unchanged, check if the HOLD function is enabled.

### 1.3. AFTER USE

- When measurement is complete, switch off the instrument.
- If the instrument is not to be used for a long time, remove the battery.

## 2. GENERAL DESCRIPTION

The instrument is a precision digital luxmeter, mainly used for measuring illuminance of both white light sources and LED sources of various colours, expressed in Lux (Lx) or Foot-candles (Fc). The instrument complies with CIE (International Commission on Illumination) standards on spectrum response and corrects according to the cosine of the angle of incidence of light. The silicon photodiode sensor guarantees measurement stability.

The instrument has the following functions:


- Illuminance measurement up to 400kLux / 40kFc
- Luminous intensity measurement (expressed in Candles)
- Selection of the measuring unit: Lx/Fc/CD
- Light source: white light source and LED sources in their visible spectrum
- High-precision and rapid measurements
- Data HOLD function
- MAX/MIN/AVG functions
- Zeroing of the displayed value
- Internal memory for saving measurement results
- Auto Power OFF
- Backlight
- Autorange

## 3. PREPARATION FOR USE

### 3.1. INITIAL CHECKS

Before shipping, the instrument has been checked from an electric as well as mechanical point of view. All possible precautions have been taken so that the instrument is delivered undamaged. However, we recommend generally checking the instrument in order to detect possible damage suffered during transport. In case anomalies are found, immediately contact the forwarding agent. We also recommend checking that the packaging contains all components indicated in § 7.3. In case of discrepancy, please contact the Dealer. In case the instrument should be returned, please follow the instructions given in § 8

### 3.2. INSTRUMENT POWER SUPPLY

The instrument is powered by a single 9V alkaline battery type NEDA1604, JIS006P, IEC6F22 included in the package. In order to prevent battery discharge, it has not been inserted in the instrument. For battery installation, follow the instructions given in § 6.1. The "" symbol appears when the battery is flat. Replace the battery by following the instructions given in § 6.1.

### 3.3. STORAGE

In order to guarantee precise measurement, after a long storage time under extreme environmental conditions, wait for the instrument to come back to normal condition (see § 7.2.1).

## 4. NOMENCLATURE

### 4.1. INSTRUMENT DESCRIPTION




**CAPTION:**

1. Input terminal
2. LCD display
3. **LX/FC/CD** key
4. **MAXMIN** key
5. **HLD** key
6. **MEM/READ** key
7. **▲** arrow key
8. **☀/SRC** key
9. **▼** arrow key
10. **ZRO** key
11. **ON/OFF** key
12. Photodiode sensor

Fig. 1: Instrument description

### 4.2. DISPLAY DESCRIPTION

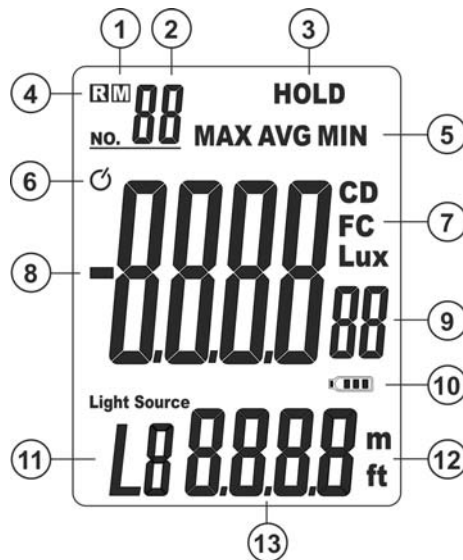

**CAPTION:**

1. **M** symbol (Memory)
2. Location number
3. **HOLD** function active
4. **R** symbol (Recall)
5. **MAX, MIN, AVG** functions active
6. **APO** function active
7. Illuminance measurement unit
8. Main display
9. Secondary display
10. Low battery indication
11. Light source type
12. Distance measurement unit
13. Source coefficient

Fig. 2: Display description

### 4.3. DESCRIPTION OF FUNCTION KEYS

#### 4.3.1. ON/OFF key

By pushing **ON/OFF** key permits to turn on and off the instrument. The same key is used also to disable the Auto Power OFF (APO) feature (see § 4.3.9).

#### 4.3.2. LX/FC/CD key

- Press the **LX/FC/CD** key to select the measuring unit of illuminance, choosing between the two available options “LUX” and “FC” ( $1\text{Fc} = 10.764\text{Lux}$  ;  $1\text{Lux} = 0.09290\text{Fc}$ ).
- Press longer **LX/FC/CD** (>1s) in order to select the measuring unit of luminous intensity (see § 5.2)

#### 4.3.3. HLD key

By pushing **HLD** key the instrument's measured value is frozen on the display and the symbol “HOLD” appears on it. The HOLD function is not active with MAX, MIN or AVG features enabled.

#### 4.3.4. MEM/READ key

- Press the **MEM/READ** key to save the datum shown on the display in the internal memory. The indication of the memory location (max. 99 locations) and the symbol “M” (see Fig. 2 – parts 1 and 2) appear for a while at the top left part of the display
- Press longer **LX/FC/CD** (>1s) allows recalling the data saved in the internal memory on the display. The symbol “R” with the number of the last memory location used are shown on the top left part of the display. Use the arrow keys ▼ or ▲ to select memory locations. The display shows the corresponding saved value. Press again longer **LX/FC/CD** (>1s) to exit the function

#### 4.3.5. Deleting the internal memory

To delete the internal memory, proceed as follows:

1. Switch off the instrument using the **ON/OFF** key.
2. Press and hold the **MEM/READ** key while switching on the instrument with the **ON/OFF** key. The messages “CLR” is shown on the display for a few seconds and the number of the memory location is taken back to “00”.




#### 4.3.6. MAXMIN key

Press the **MAXMIN** key to view the Minimum, Maximum and Average (AVG) values of the measured quantity. The values are constantly updated and are displayed cyclically every time the same key is pressed. The symbols “MIN”, “MAX” and “AVG” appear on the display. Press longer **MAXMIN** (>1s) to exit the function.

#### 4.3.7. ZRO key


Press the **ZERO** key to carry out the automatic zeroing of the value on the display in case the indication “000” should be absent when placing the protection cover onto the photodiode sensor. The message “Adj” is shown on the display during this operation. The message “CAP” is shown on the display in case the **ZRO** key is pressed with the protection cover not positioned on the sensor. Insert the cover and repeat the operation, if necessary.

#### 4.3.8. /SRC (Light Source) key


- Press the /SRC key to active/disable tye display backlight
- Press longer /SRC (>1s) key in order to select the light source to be measured. Proceed as follows:
  1. On the sub-display, observe the flashing symbol “Lx”, where  $0 < x < 9$  indicates the source number.
  2. Use the arrow keys ▲ or ▼ to select the desired source among the available options L0 ÷ L9 (see Table 1)
  3. Press the /SRC key to set a possible correction factor on the instrument’s reading (only for custom sources L7, L8 and L9). The indication of the parameter value flashes on the display. Use the arrow keys ▲ or ▼ to set (press and hold the keys for rapid operation) the value between **0.001** and **1.999**. The values of the sources L0 ÷ L5 cannot be modified


Symbol on the display	Source type	Correction factor
L0	Standard light	1.000
L1	White LED	0.990
L2	Red LED	0.516
L3	Yellow LED	0.815
L4	Green LED	1.216
L5	Blue LED	1.475
L6	Purple LED	1.148
L7	Custom	1.000
L8	Custom	1.000
L9	Custom	1.000

Table 1: List of available sources

4. Press longer /SRC (>1s) to confirm the operation. The symbols stop flashing on the display.

#### 4.3.9. Disabling the Auto Power OFF function

In order to preserve the instrument’s internal battery, the instrument switches automatically off approximately 5 minutes after it was last used. The symbol “” appears on the display. To disable the Auto Power Off function, proceed as follows:

- Switch on the instrument.
- Press longer **ON/OFF** key (>1s). The symbol “” disappears from the display
- Press again longer **ON/OFF** key (>1s) or switch off and then on again the instrument to automatically enable the function

## 5. OPERATING INSTRUCTIONS

### 5.1. ILLUMINANCE MEASUREMENT

1. Insert the protection cover onto the photodiode sensor.
2. Switch on the instrument using the **ON/OFF** key.
3. If necessary, zero the display by pressing the **ZRO** key (see § 4.3.7).
4. Select the measuring unit Lux or Fc on the instrument by pressing the **LX/FC/CD** key (see § 4.3.2).
5. Select the type of source to be tested by pressing and holding the **☀/SRC** key for more than 1 second (see § 4.3.8). Standard source is type "L0".
6. Position the sensor horizontally and perpendicularly with respect to the source to be tested. The illuminance value is shown on the display, with automatic scale change.
7. Press the **HLD** key, if necessary (see § 4.3.3) to freeze the value shown on the display.
8. Press the **MEM/READ** key (see § 4.3.4) to save the datum, read in real time and shown on the display, in the memory.
9. Cover the sensor and switch off the instrument at the end of measurement.

### 5.2. LUMINOUS INTENSITY MEASUREMENT

Luminous intensity, expressed in Candles (CD), is calculated by the instrument according to the following formula:

$$\text{Luminous intensity (CD)} = \text{Illuminance (Lux/Fc)} \times \text{Distance from source (m}^2\text{/ft}^2\text{)}$$

1. Insert the protection cover onto the photodiode sensor.
2. Switch on the instrument using the **ON/OFF** key.
3. If necessary, zero the display by pressing the **ZRO** key (see § 4.3.7).
4. Select the measuring unit on the instrument by pressing longer (1s) LX/FC/CD key. The symbol "CD" is shown on the display.
5. Use the arrow keys **▲** or **▼** to select the measuring unit of distance "m" or "ft" (see Fig. 2 – part 12) and confirm with **LX/FC/CD**
6. Select the type of source to be tested by pressing and holding the **☀/SRC** key for more than 1 second (see § 4.3.8). Standard source is type "L0"
7. Set the value of the distance between the measured point and the light source using the arrow keys **▲** or **▼** in the ranges **0.01m ÷30.347m** or **0.01ft ÷99.99ft** and confirm with the **LX/FC/CD** key
8. Position the sensor horizontally and perpendicularly with respect to the source to be tested. The value of luminous intensity is shown on the display, with automatic scale change.
9. Press the **HLD** key, if necessary (see § 4.3.3) to freeze the value shown on the display.
10. Press the **MEM/READ** key (see § 4.3.4) to save the datum, read in real time and shown on the display, in the memory.
11. Cover the sensor and switch off the instrument at the end of measurement.



## 6. MAINTENANCE

### CAUTION



- Only expert and trained technicians should perform maintenance operations. Before carrying out maintenance operations, disconnect all cables from the input terminals.
- Do not use the instrument in environments with high humidity levels or high temperatures. Do not expose to direct sunlight.
- Always switch off the instrument after use. In case the instrument is not to be used for a long time, remove the battery to avoid liquid leaks that could damage the instrument's internal circuits.

### 6.1. BATTERY REPLACEMENT

When the display shows the " symbol, replace the battery.

1. Switch off the instrument
2. Remove the temperature probe
3. Remove the battery cover
4. Remove the battery from the battery fastener
5. Set the new battery into battery fastener, and return it to the battery case
6. Replace the battery cover
7. Use the appropriate battery disposal methods for Your area.

### 6.2. CLEANING THE INSTRUMENT

Use a soft and dry cloth to clean the instrument. Never use wet cloths, solvents, water, etc. The white plastic lens of the sensor may be cleaned, if necessary, with a wet cloth.

### 6.3. END OF LIFE



**CAUTION:** the symbol on the instrument indicates that the appliance, the battery and its accessories must be collected separately and correctly disposed of.

## 7. TECHNICAL SPECIFICATIONS

### 7.1. TECHNICAL CHARACTERISTICS

Accuracy is referred to the following reference conditions: temperature 25°C (77°F) with relative humidity < 70%RH

The instrument is calibrated for a standard white light source consisting of an incandescent lamp, at a temperature/colour of 2856°K in compliance with Class A.

Calibration for LED sources (with spectrum response different from that of standard white light) is based on the calibration for standard white light source in Class A using the appropriate correction factors (see Table 1)

#### Illuminance measurement (Aurorange)

Full scale (Lux)	40	400	4000	40k	400k
Resolution (Lux)	0.01	0.1	1	10	100
Accuracy	± (3%reading)				

Full scale (Fc)	40	400	4000	40k
Resolution (Fc)	0.01	0.1	1	10
Accuracy	± (3%reading)			

NOTE 1: 1Fc=10.76Lux, 1Klux=1000Lux, 1Kfc=1000Fc

NOTE 2: for temperature/colours different from the reference one, accuracy becomes 6%reading

Distance range for luminous intensity measurement: 0.01 ÷ 30.47m / 0.01 ÷ 99.99ft

Accuracy on angular deviation from cosine characteristic	
30°	± 2%
60°	± 6%
80°	± 25%

#### 7.1.1. Spectrum response

The spectrum response of the photodiode with filter is almost identical to the CIE photo-optical curve  $V(\lambda)$  as shown in the following graph.

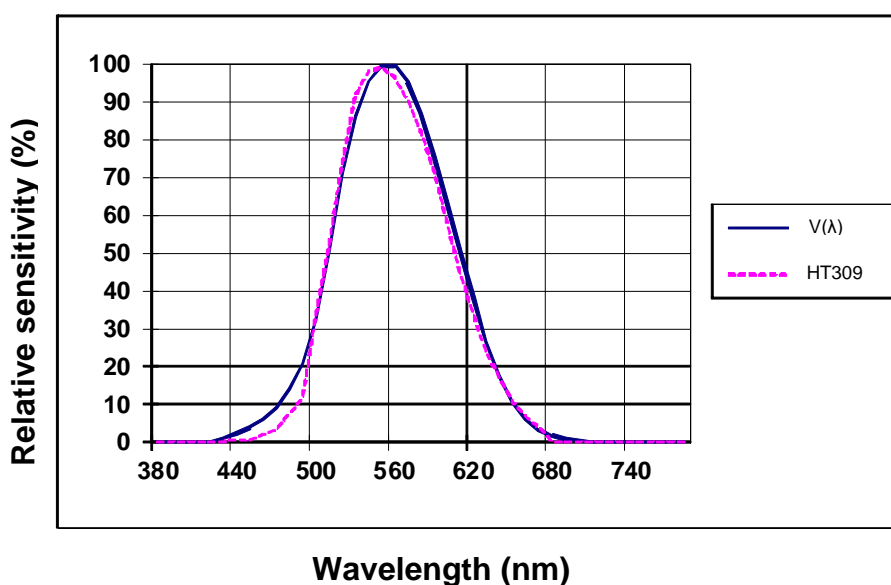


Fig. 2: CIE curve  $V(\lambda)$ .

#### 7.1.2. Sensor


The sensor is a silicon photodiode with filter on the spectrum response.

### 7.1.3. General characteristics

#### Mechanical characteristics

Dimensions (L x W x H):	190 x 65 x 45mm (7 x 3 x 2in)
Sensor dimensions (L x W x H):	110 x 60 x 35mm (4 x 2 x 1in)
Cable length:	approx 1.5m (39in)
Weight (battery included):	235g (8 ounces)

#### Power supply

Battery type:	1x9V battery type NEDA 1604 IEC 6F22
Low battery indication:	the display shows symbol "  "
Battery life:	ca 60h (backlight ON), ca 180h (backlight OFF)

#### Display

Characteristics:	LCD, 6 digits, 4000 dots plus decimal point
Over range indication:	the display shows symbol "OL"
Sampling rate:	2.5 measurements/s

#### Considered standards

EMC:	IEC/EN61326-1, IEC61000-4-2, IEC61000-4-3
Reference standard:	JIS C 1609:1993 and CNS 5119 general specification in Class A
Pollution level:	2

## 7.2. ENVIRONMENT

### 7.2.1. Environmental conditions for use

Reference temperature:	25°C (77°F)
Operating temperature:	5°C ÷ 40°C (41°F ÷ 104°F)
Allowable relative humidity:	<80%RH
Storage temperature:	-10°C ÷ 60°C (14°F ÷ 140°F)
Storage humidity:	<70%RH
Max operating altitude:	2000m (6562ft)

**This instrument satisfies the requirements of EMC Directive 2014/30/EU  
This instrument satisfies the requirements of European Directive 2011/65/EU (RoHS)  
and 2012/19/EU (WEEE)**

## 7.3. ACCESSORIES

### 7.3.1. Accessories provided

- Carrying bag
- Battery (not inserted)
- User manual

## 8. SERVICE

### 8.1. WARRANTY CONDITIONS

This instrument is warranted against any material or manufacturing defect, in compliance with the general sales conditions. During the warranty period, defective parts may be replaced. However, the manufacturer reserves the right to repair or replace the product. Should the instrument be returned to the After-sales Service or to a Dealer, transport will be at the Customer's charge. However, shipment will be agreed in advance. A report will always be enclosed to a shipment, stating the reasons for the product's return. Only use original packaging for shipment; any damage due to the use of non-original packaging material will be charged to the Customer. The manufacturer declines any responsibility for injury to people or damage to property.

The warranty shall not apply in the following cases:

- Repair and/or replacement of accessories and batteries (not covered by warranty).
- Repairs that may become necessary as a consequence of an incorrect use of the instrument or due to its use together with non-compatible appliances.
- Repairs that may become necessary as a consequence of improper packaging.
- Repairs which may become necessary as a consequence of interventions performed by unauthorized personnel.
- Modifications to the instrument performed without the manufacturer's explicit authorization.
- Use not provided for in the instrument's specifications or in the instruction manual.

The content of this manual cannot be reproduced in any form without the manufacturer's authorization.

**Our products are patented and our trademarks are registered. The manufacturer reserves the right to make changes in the specifications and prices if this is due to improvements in technology.**

### 8.2. SERVICE

If the instrument does not operate properly, before contacting the After-sales Service, please check the conditions of the battery and replace it, if necessary. Should the instrument still operate improperly, check that the product is operated according to the instructions given in this manual. Should the instrument be returned to the After-sales Service or to a Dealer, transport will be at the Customer's charge. However, shipment will be agreed in advance. A report will always be enclosed to a shipment, stating the reasons for the product's return. Only use original packaging for shipment; any damage due to the use of non-original packaging material will be charged to the Customer.